

Instruction Manual
DULCOMETER® 2201 X Cond

ProMinent®



ProMinent Dosiertechnik GmbH • D-69123 Heidelberg • Germany

ProMinent Dosiertechnik GmbH
Im Schuhmachergewann 5–11
D-69123 Heidelberg
Postfach 10 17 60
D-69007 Heidelberg
Telephone: +49 (06221) 842-0
Fax: +49 (06221) 842-419
info@prominent.de
www.prominent.de



We reserve the right to make technical changes.

TA-194.200-PME01 290601

Software Version: 1.x

Safety Precautions

Be sure to read and observe the following requirements!

The DULCOMETER® 2201 X Cond is approved for operation in hazardous locations.

Warning  Before connecting the device to a power supply unit, make sure that this is an associated apparatus.

Whenever it is likely that the protection has been impaired, the device shall be made inoperative and secured against unintended operation.

The protection is likely to be impaired if, for example:

- the device shows visible damage
- the device fails to perform the intended measurements
- after prolonged storage at temperatures above 70 °C
- after severe transport stresses

Before recommissioning the device, a professional routine test in accordance with EN 61010-1 must be performed. This test should be carried out at our factory.

The device shall not be used in a manner not specified by this manual.

Information on this Instruction Manual

ITALICS are used for texts which appear in the display.

Bold print is used to represent keys, e.g. **cal**.



Keys for which the functions are explained are frequently shown in the left-hand column.

Note



Notes provide important information that should be strictly followed when using the device.

Warning



Warning means that the instructions given must always be followed for your own safety. Failure to follow these instructions may result in injuries.

Mode Codes

After pressing **cal** or **conf** you can enter one of the following codes to access the designated mode:



conf, 0000: Error info
conf, 1200: Configuration
conf, 5555: Current source



cal, 0000: Cal info
cal, 1015: Temp probe adjustment
cal, 1100: Calibration mode
cal, 2222: Test mode

Contents

| | | | |
|---|-----------|--|-----------|
| Safety Precautions | 3 | 4 Diagnostics, Maintenance and Cleaning | 23 |
| Information on this Instruction Manual ... | 4 | Sensoface®, Sensocheck® | 23 |
| Mode Codes | 4 | Error Messages | 23 |
| 1 Assembly | 6 | Diagnostics Functions | 25 |
| Package Contents and Unpacking | 6 | Maintenance and Cleaning | 26 |
| Assembly | 6 | 5 Appendix | 27 |
| 2 Installation, Connection and Commissioning | 10 | Product Line | 27 |
| Proper Use | 10 | Specifications | 28 |
| Overview of DULCOMETER® 2201 X Cond | 10 | EC-Type-Examination Certificate | 30 |
| Terminal Assignment | 11 | Declaration of Conformity | 33 |
| Installation and Commissioning | 11 | Sensors | 34 |
| Typical Wiring | 12 | Calibration Solutions | 36 |
| 3 Operation | 13 | Index | 37 |
| User Interface | 13 | | |
| Display | 14 | | |
| Keypad | 14 | | |
| Safety Functions | 15 | | |
| Outputs | 16 | | |
| Configuration | 17 | | |
| Calibration | 19 | | |
| Measurement | 22 | | |

1 Assembly

Package Contents and Unpacking


Unpack the device carefully and check the shipment for transport damage and completeness.
The package contains:

- Front unit of DULCOMETER® 2201 X Cond
- Lower case
- Short instruction sheet
- This instruction manual

- Bag containing:

- | | |
|----------------------|------------------|
| ① 2 sealing plugs | ⑦ 1 hinge pin |
| ② 5 hexagon nuts | ⑧ 3 cable ties |
| ③ 3 cable glands | ⑨ 3 filler plugs |
| ④ 1 rubber reducer | ⑩ 3 gaskets |
| ⑤ 1 sealing insert | ⑪ 1 washer |
| ⑥ 4 enclosure screws | ⑫ 1 jumper |

Assembly

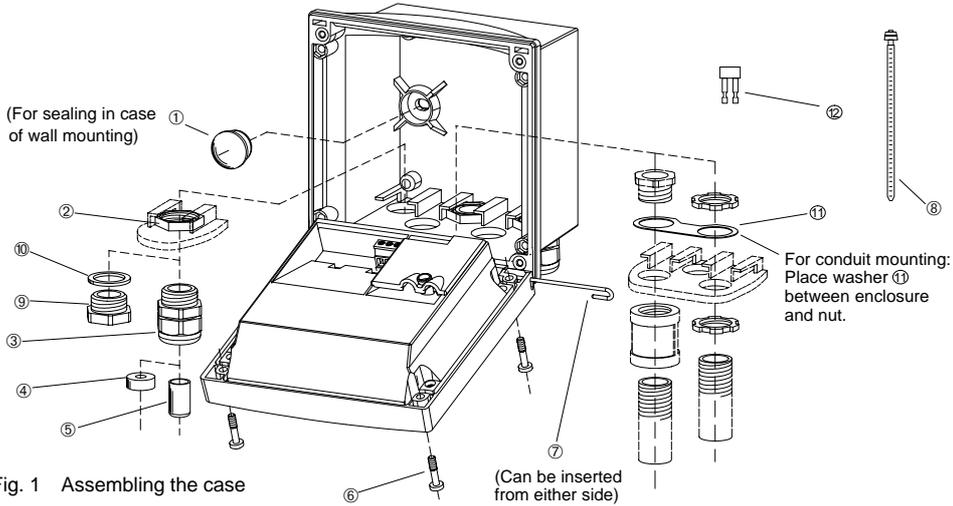

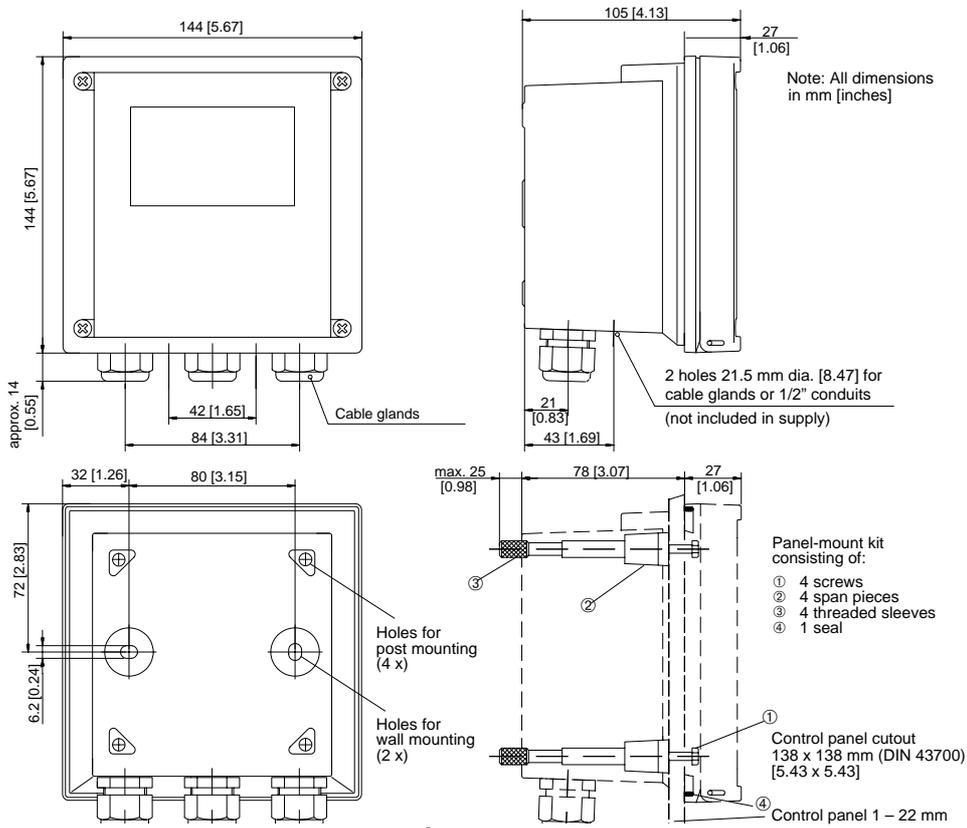


Fig. 2 Dimension drawing for DULCOMETER® 2201 X Cond, mounting diagram and panel-mount kit (Order No. 1008708)

Pipe-mount kit
consisting of:

- ① 4 self-tapping screws
- ② 1 post mounting plate
- ③ 2 hose clamps with
worm gear drive
to DIN 3017

For vertical or
horizontal post/
pipe mounting

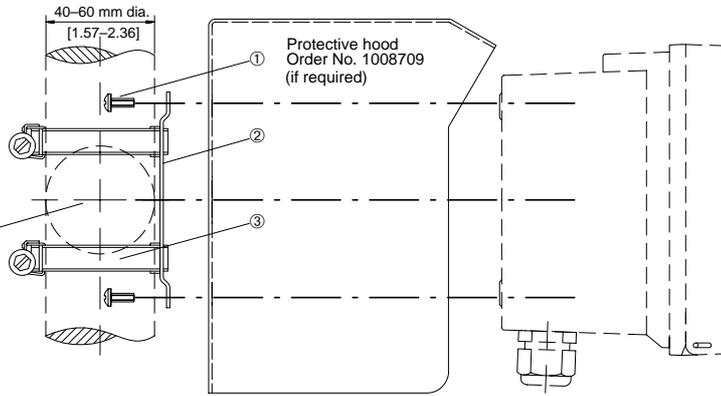


Fig. 3 Pipe-mount kit (Order No. 1008707)

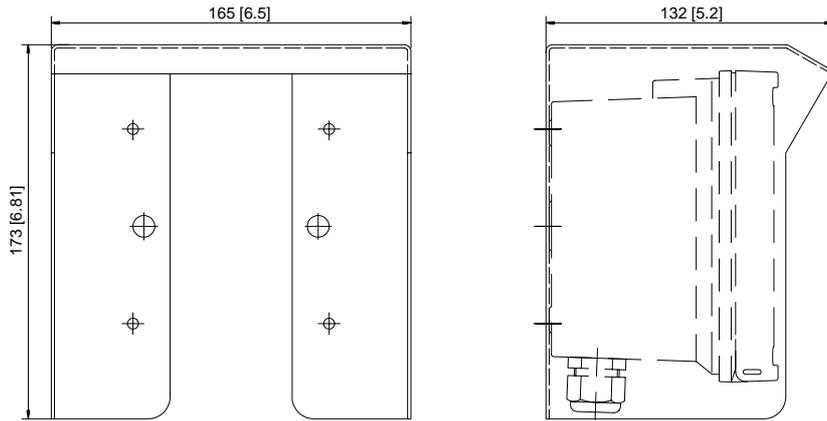


Fig. 4 Protective hood (Order No. 1008709) for wall and pipe mounting

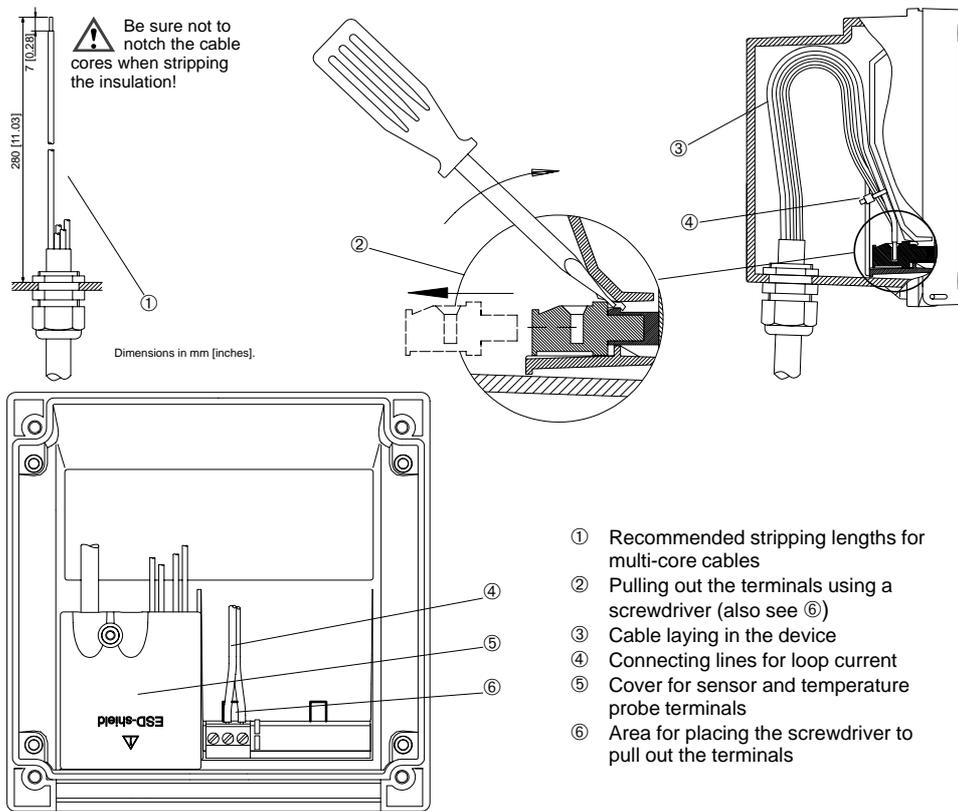


Fig. 5 Installation information DULCOMETER® 2201 X Cond

2 Installation, Connection and Commissioning

Proper Use

DULCOMETER[®] 2201 X Cond is used for conductivity and temperature measurement in biotechnology, food processing, pharmaceutical and chemical industry, waste-water treatment, as well as for monitoring ultrapure water. It can be either field-mounted or fixed into a control panel.



DULCOMETER[®] 2201 X Cond is approved for operation in hazardous locations.

Overview of DULCOMETER[®] 2201 X Cond

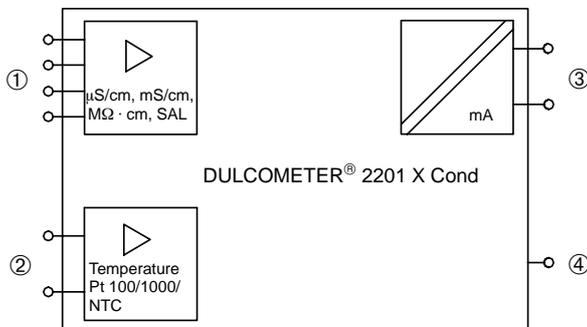


Fig. 6 System functions of DULCOMETER[®] 2201 X Cond

- ① Inputs for 2-/4-electrode cond. sensor
- ② Input for temperature probe
- ③ Current loop 4 – 20 mA
- ④ Equipotential bonding

Terminal Assignment

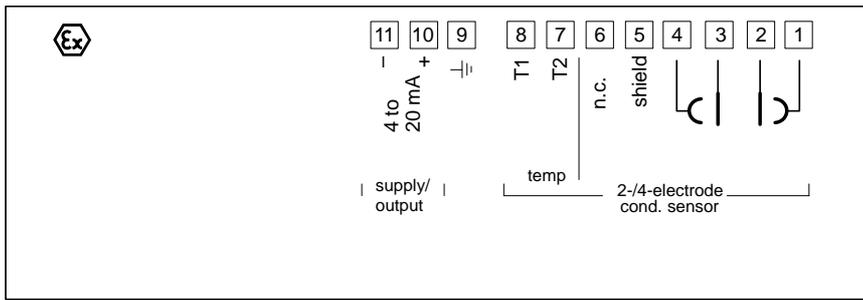


Fig. 7 Terminal assignment of DULCOMETER® 2201 X Cond

Installation and Commissioning

Warning  *Installation and commissioning of the DULCOMETER® 2201 X Cond may only be carried out in accordance with this instruction manual and per applicable local and national codes. Be sure to observe the technical specifications and input ratings.*

Warning  Do not use alternating current or mains power supply!

Warning  DULCOMETER® 2201 X Cond may only be connected to an explosion-proof power supply unit (for input ratings refer to schedule of Type Examination Certificate).

Warning  When commissioning, a complete configuration must be carried out.

Warning  For easier installation, the terminal strips are of a plug-in design. The terminals are suitable for single wires and flexible leads up to 2.5 mm² (AWG 14) (see Pg. 9). See Pg. 12 for a connection example.

Typical Wiring

Conductivity measurement with LF 604 2-electrode cell

The LF 604 2-electrode cell is used for measuring conductivity values from 0 to 1000 $\mu\text{S}/\text{cm}$.

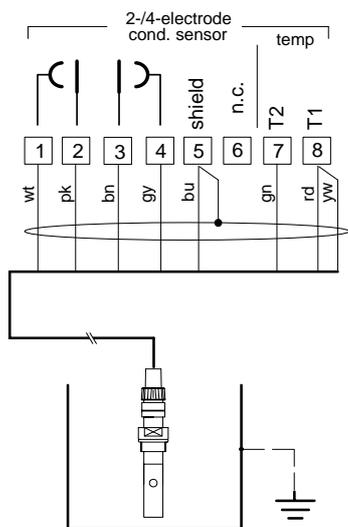


Fig. 8 Conductivity measurement with LF 604 2-electrode cell

Settings for LF 604 2-electrode cell

| | Menu | Setting |
|------------------------|-----------|---------|
| Meas. procedure | conf 1200 | 2-EL |
| Temp probe | conf 1200 | Pt 1000 |
| Cell constant | cal 1100 | 0.0290 |

3 Operation

User Interface

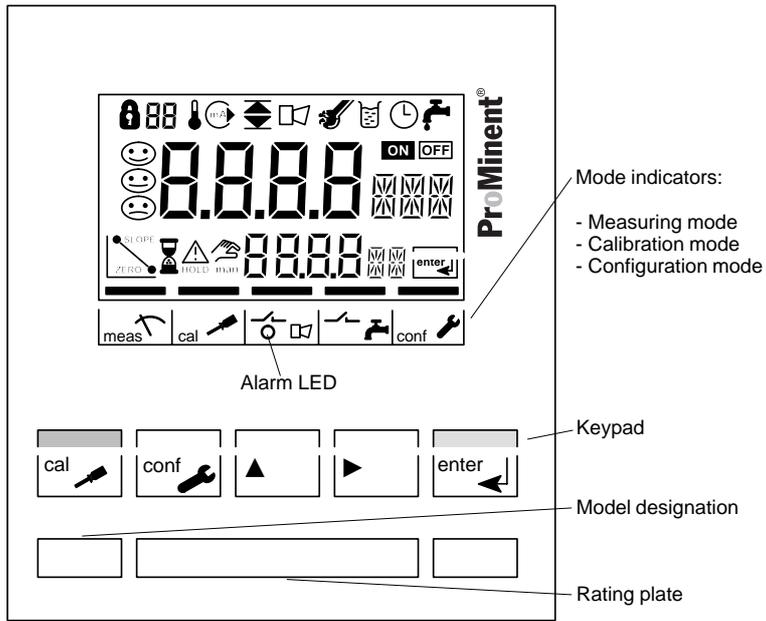


Fig. 9 Front view of DULCOMETER® 2201 X Cond

Display

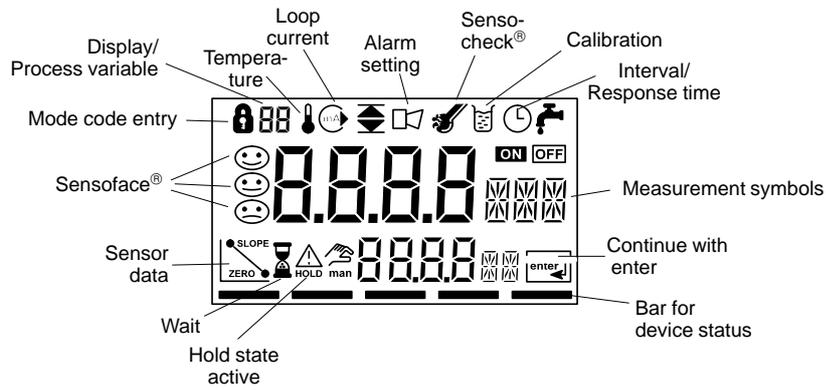


Fig. 10 Display

Keypad

| | | | |
|--|--|---|---|
|  | Start, end calibration |  | <u>Prompt in display:</u> continue in program sequence, <u>Configuration:</u> Confirm entries, next configuration step, <u>Measuring mode:</u> Display loop current |
|  | Start, end configuration | | |
|  | Select digit position (selected position flashes) |  →  | Cal info, display cell constant (see Pg. 22) |
|  | Change digit |  →  | Error info, display last output error message (see Pg. 22) |
| | |  +  | Start GainCheck® manual device self-test (see Pg. 15) |

Safety Functions

Sensoface® sensor monitoring



Sensoface® provides information on the sensor condition. A sad “Smiley” indicates that there is a Sensocheck® message.

Sensocheck® alerts for significant sensor polarization or excessive cable capacitance caused by an unsuitable cable or a cable that is too long. Sensocheck® can be switched off. With Sensocheck® switched off, no friendly Smiley appears.

For more detailed information, see chapter “Diagnostic, Maintenance and Cleaning” (Pg. 23).

GainCheck® manual device self-test



Simultaneously pressing ▲ and ► starts the manual device self-test.

A display test is carried out, the software version is displayed and the memory and measured value transmission are checked.

Automatic device self-test

The automatic device self-test checks the memory and the measured-value transmission. It runs automatically in the background at fixed intervals.

Outputs

Current loop (4 to 20 mA)

The current is controlled by the process variable selected in the configuration.

The current characteristic can be configured as linear or logarithmic curve for conductivity and resistivity.

The current beginning and end can be set to represent any desired value.

If LIN (linear characteristic) is chosen, the minimum span is 5% of the selected process variable / measurement range. If LOG (logarithmic characteristic) is chosen, the minimum span is one decade within the chosen range.

To check connected peripherals (e.g. limit switches, controllers), the loop current can be manually specified (see Pg. 25).

Alarm

During an error message the alarm LED flashes. Alarm response time is permanently set to 10 sec.

Error messages can also be signaled with a 22 mA signal via the loop current (see Configuration, Pg. 18).

Configuration

The device arrives from the factory configured and ready to operate as a conductivity transmitter. This section provides detailed procedures for changing operation values for specific applications.



Activate with **conf** change parameter with ▲ and ►, confirm/continue with **enter**, end with **conf**.



Mode code "1200"








During configuration the device is in the Hold state, the loop current is frozen.



Note The configuration parameters are checked during the input. In the case of an incorrect input "ERR" is displayed for 3 sec. The parameters cannot be stored with **enter** until the input has been repeated.

Configuration parameters

| Picto-graph | Parameter | Choices | Factory setting |
|-------------|---|---|-------------------------|
| | Sensor selection | 2-EL (2-electrode cell) 4-EL (4-electrode cell) | 2-electrode cell |
| | Process variable / meas. range Selected process variable and measuring range control loop current and measured values. Complete configuration required after change. | 0.000 µS / 00.00 µS / 000.0 µS / 0000 µS 0.000 mS / 00.00 mS / 000.0 mS 0.000 MΩ / 00.00 MΩ / 000.0 MΩ 0.000 SAL | 000.0 mS |
| | Temperature display | °C °F | °C |
| | Temperature probe | Pt 100 / Pt 1000 / NTC 30 kΩ / NTC 100 kΩ | Pt 100 |

| | | | |
|---|---|---|-----------|
|  tc | Temperature compensation (not with SAL) | OFF LIN NLF (natural waters) -01- FCT (ultrapure water, NaCl traces) -02- FCT (ultrapure water, HCl traces) -03- FCT (ultrapure water, NH ₃ traces) | OFF |
|  tc | Temperature coefficient (only with tc LIN) | xx.xx %/K | 02.00 %/K |
|  mA 0.00 | Current characteristic (not with SAL) | LIN LOG | LIN |
|  mA 4.00 | Current beginning (0 / 4 mA) (only with LIN) | μS / mS / MΩ / SAL | 000.0 mS |
|  mA 20.00 | Current end (20 mA) (only with LIN) | μS / mS / MΩ / SAL | 100.0 mS |
|  mA 4.00 | Current beginning (0 / 4 mA) (only with LOG) | μS / mS / MΩ * | 0.1 mS |
|  mA 20.00 | Current end (20 mA) (only with LOG) | μS / mS / MΩ * | 100 mS |
|  mA HOLD | Hold state | Last: Last current value Fix: Current specified | Last |
|  mA F 21.00 | Hold value (only with Fix) | xx.xx mA | 21.00 mA |
|  22 mA | 22 mA signal for error message | ON / OFF | OFF |
|  CHECK | Sensocheck® | ON / OFF | OFF |

* 0.1 / 1 / 10 / 100 / 1000 μS / mS / MΩ

Configuration is circular. To stop, press **conf.**

Calibration

In the calibration mode the cell constant can be changed in two ways. If the cell constant of the cell in use is known, it can be entered directly. Furthermore, the cell constant can be determined with a known calibration solution under consideration of the temperature.



Activate with **cal**, confirm/continue with **enter**, abort with **cal** → **enter**



During calibration the device is in the Hold state. The loop current is frozen.

When the calibration mode is exited, the device remains in the Hold state for safety reasons. This prevents undesirable reactions of the connected peripherals (e.g. limit switches, controllers) due to incorrect settings. The measured value and *Hold* are displayed alternately. Now you can check whether the measured value is plausible and specifically end the Hold state with **enter** or repeat calibration with **cal**. If you end the Hold state, the device will return to measuring mode after 20 sec (measured value stabilization).

Calibration by input of cell constant



Activate calibration by pressing the **cal** key. Using the ▲, ► keys enter mode code "1100" and then press **enter**.



Using the ▲, ► keys enter the cell constant. The lower display shows the conductivity value.

1000 c
99.6 µS

A change in the cell constant also changes the conductivity value.

1007 c
100.3 µS

When there has not been an entry for approx. 6 sec, conductivity and temperature are displayed alternately.

1007 c
25.1 °C



Press **enter** to confirm the cell constant.

Hold

The device remains in the Hold state. You can end the Hold state with **enter**. After 20 sec (measured value stabilization) the device returns to measuring mode.

25.1 °C

Calibration with calibration solution

Note



Be sure to use known calibration solutions and the respective temperature-corrected table values (see Calibration Solutions, Pg. 38).



Activate calibration by pressing the **cal** key. Using the **▲**, **▶** keys enter mode code "1100" and then press **enter**.



Immerse the conductivity cell in the calibration solution.



After approx. 6 sec the lower display alternately shows the conductivity and temperature values. Read the conductivity value corresponding to the displayed temperature from the table of the used calibration solution (for tables see Pg. 38).



Using the **▲**, **▶** keys change the cell constant until the display shows the conductivity value from the table.



Make sure that the temperature is stable during the calibration procedure.



Press **enter** to confirm the cell constant.

Hold



The device remains in the Hold state. You can end the Hold state with **enter**. After 20 sec (measured value stabilization) the device returns to measuring mode.

Adjustment of temperature probe

Note  This function should only be used by experts. Incorrectly set parameters may go unnoticed, but change the measuring properties. Especially for Pt 100 temperature probe, it is advisable to perform an adjustment.



Activate calibration by pressing the **cal** key.



Using the ▲, ► keys enter mode code "1015" and then press **enter**.



Measure the temperature of the process medium using an external thermometer.



Using the ▲, ► keys enter the determined temperature value in the main display. If you take over the temperature value shown in the lower display, the correction is without effect.



Press **enter** to confirm the temperature value.



The device remains in the Hold state. You can end the Hold state with **enter**. After 20 sec (measured value stabilization) the device returns to measuring mode.

Measurement

Measuring mode

In the measuring mode the main display shows the configured process variable and the lower display the temperature.

Cal info

With **cal** and mode code "0000" you can activate the cal info. Cal info shows the current calibration data for approx. 20 sec. The 20 sec can be reduced by pressing **enter**. During cal info the device is not in Hold state.

Error info

With **conf** and mode code "0000" you can activate the error info. Error info shows the most recent error message for approx. 20 sec. After that the message will be deleted. The 20 sec can be reduced by pressing **enter**. During error info the device is not in Hold state.

Hold state

The device will enter the Hold state under the following conditions:



For calibration: Mode code 1015
Mode code 1100
Mode code 2222

configuration: Mode code 1200
Mode code 5555

The loop current is frozen at *Last* or *Fix* (configuration Pg. 18).

If the calibration or configuration mode is exited, the device remains in the Hold state for safety reasons. This prevents undesirable reactions of the connected peripherals (e.g. limit switches, controllers) due to incorrect settings. The measured value and *Hold* are displayed alternately. Now you can check whether the measured value is plausible and specifically end the Hold state with **enter**. After 20 sec (for the measured value stabilization) the device returns to measuring mode.

Note



During error conditions the Hold state will not be active.

4 Diagnostics, Maintenance and Cleaning

Sensoface®, Sensocheck®



Sensoface® provides information on the sensor condition. A sad “Smiley” indicates that there is a Sensocheck® message.



Sensocheck® alerts for significant sensor polarization or excessive cable capacitance caused by an unsuitable cable or a cable that is too long. Sensocheck® can be switched off. With Sensocheck® switched off, no friendly Smiley appears.

Error Messages

When one of the following error messages is output, the device can no longer correctly determine the process variable or output it via the loop current.

During an error message the alarm LED flashes. The alarm response time is permanently set to 10 sec.

Error messages can also be signaled with a 22 mA signal via the loop current (see Configuration, Pg. 18).

Error info



With **conf** and mode code “0000” you can activate the error info. Error info shows the most recent error message for approx. 20 sec. After that the message will be deleted. The 20 sec can be reduced by pressing **enter**. During error info the device is not in Hold state.

| Error number | Display (flashing) | Problem | Possible causes |
|--------------|--------------------|-------------------|---|
| Err 01 | 1179 mS/cm | Conductivity cell | - Wrong cell constant - Conductivity \geq 1000 mS/cm - SAL > 45 ‰ - Cell connection or cable defective |
| Err 02 | | Conductivity cell | - Unsuitable cell |
| Err 03 | | Temperature probe | - Outside temp range - Outside temp range for TC - Outside temp range for SAL |
| Err 21 | | Loop current | - Meas. value below configured current beginning - Wrong configuration for current beginning (see Pg. 18) |

| Error number | Display (flashing) | Problem | Possible causes |
|--------------|---|-------------------------|--|
| Err 22 |  | Loop current | - Meas. value above configured current end - Wrong configuration for current end (see Pg. 18) |
| Err 23 |  | Loop current | - Configured current span too small (Difference between current beginning and end) |
| Err 33 |  | Sensocheck [®] | - Wrong conductivity cell - Conductivity cell defective - Connection cable or screw cap defective - Connection terminals or screw cap dirty |
| Err 98 | CONF | System error | - Configuration or calibration data defective; completely reconfigure and recalibrate the device - Measured value transmission defective - Memory error in device program (PROM defective) |
| Err 99 | FAIL | Factory settings | - EEPROM or RAM defective - Error in factory settings This error message normally should not occur, as the data are protected from loss by multiple safety functions. Should this error message nevertheless occur, there is no remedy. The device must be repaired and recalibrated at the factory. |

Diagnostics Functions

Cal info

Pressing **cal** and entering mode code "0000" is going to activate the cal info. Cal info shows the current calibration data for approx. 20 sec. During cal info the device is not in Hold state.

Test mode

Pressing **cal** and entering mode code "2222" is going to activate the test mode. In the test mode you can check the measuring equipment with a resistor. Sensoface® is disabled. The resistor is connected instead of the conductivity cell. The equivalent resistance value is shown in the main display in kΩ. With a resistance value > 2 MΩ the display reads "OPEN". Pressing **enter** ends the test mode. The device goes to Hold state.

Error info

Pressing **conf** and entering mode code "0000" is going to activate the error info. Error info shows the most recent error message for approx. 20 sec. After that the message will be deleted. During error info the device is not in Hold state.

Display loop current

Pressing **enter** in measuring mode displays the loop current for a few seconds.

Current source

To check the connected peripherals (e.g. limit switches, controllers), the loop current can be manually specified.

Warning



In the current source mode the loop current no longer follows the measured value! It is manually specified.

Therefore, it must be ensured that the connected devices (control room, controllers, indicators) do not interpret the current value as a measured value!

Pressing **conf** and entering mode code "5555" is going to activate the current source mode. Specify the loop current using **▶**, **▲** and **enter**. The actually flowing loop current is shown in the lower display. Pressing **conf** exits the current source mode again.

GainCheck® manual device self-test

The manual device self-test is started by simultaneously pressing **▲** and **▶**.

A display test is carried out, the software version is displayed and internal functions are checked.

Automatic device self-test

The automatic device self-test checks the memory and the measured-value transmission. It runs automatically in the background at fixed intervals.

Maintenance and Cleaning

Maintenance

DULCOMETER® 2201 X Cond contains no user repairable components.

Cleaning

To remove dust, dirt and spots, the external surfaces of the device may be wiped with a damp, lint-free cloth. A mild household cleaner may also be used if necessary.

5 Appendix

Product Line

Device

| | Ref. No. |
|--|-----------------|
| DULCOMETER® 2201 X Cond for application in hazardous areas | 1008704 |

Mounting Accessories

| | Ref. No. |
|-----------------|-----------------|
| Pipe-mount kit | 1008707 |
| Panel-mount kit | 1008708 |
| Protective hood | 1008709 |

Suggested Power Supplies

| | Ref. No. |
|-----------------------|-----------------|
| Repeater power supply | |
| 90 - 253 Vac | 1008721 |
| 24 Vac/dc | 1008722 |

Specifications

| | | | | |
|--|--|--|---|---|
| Cond input | Input for 2-/4-electrode cells | Temperature compensation¹⁾ | LIN | 00.00 to 19.99 %/K |
| Display range | 0.2 $\mu\text{S} \cdot \text{cm}$ to 1000 $\text{mS} \cdot \text{cm}$ | (Ref. temp 25 °C) | NLF | Natural waters to EN 27888 (0 to 36 °C) |
| Meas. error ¹⁾ | < 1 % of meas. value \pm 0.4 $\mu\text{S} \cdot \text{cm}$ | | -01- | Ultrapure water with NaCl traces (0 to 120 °C) |
| Process variable/range | 0.000 to 9.999 $\mu\text{S}/\text{cm}$ | | -02- | Ultrapure water with HCl traces (0 to 120 °C) |
| (display resolution 3 1/2 digits) | 00.00 to 99.99 $\mu\text{S}/\text{cm}$ | | -03- | Ultrapure water with NH_3 traces (0 to 120 °C) |
| | 000.0 to 999.9 $\mu\text{S}/\text{cm}$ | | | |
| | 0.000 to 9.999 mS/cm | | | |
| | 000.0 to 999.9 mS/cm | | | |
| | 0.000 to 9.999 $\text{M}\Omega/\text{cm}$ | | | |
| | 00.00 to 99.99 $\text{M}\Omega/\text{cm}$ | | | |
| | 000.0 to 999.9 $\text{M}\Omega/\text{cm}$ | | | |
| Salinity | 0.0 to 45.0 ‰ (0 to 35 °C) | Display | LC display, alarm LED | |
| Cell monitoring | Sensocheck [®] : polarization detection and monitoring of cable capacitance (can be switched off) | Loop current | 4 to 20 mA, floating | |
| Cell standardization^{*)} | – Entry of cell constant with display of conductivity and temperature – Temperature probe adjustment | EEx ib IIC | 22 mA for error message ^{*)} supply voltage 14 to 30 V, $I_{\text{max}} = 100 \text{ mA}$, $P_{\text{max}} = 0.8 \text{ W}$ | |
| Perm. cell constant | 0.0050 to 1.9999 cm^{-1} | Characteristic ^{*)} | Linear or logarithmic | |
| Temperature input | Pt 100 / Pt 1000 / NTC 30 $\text{k}\Omega$ / NTC 100 $\text{k}\Omega$ | Current error | < 0.3 % of current value \pm 0.05 mA | |
| Ranges | – NTC –20.0 to +130.0 °C –4 to +266 °F – Pt –20.0 to +150.0 °C –4 to +302 °F | Start/End of scale^{*)} | As desired within ranges for μS , mS, $\text{M}\Omega$, SAL | |
| Resolution | 0.1 °C / 1 °F | Min. span | LIN | 5 % of selected range |
| Accuracy | < 0.5 K^2 | | LOG | 1 decade |
| | | Current source | 3.8 mA to 22.00 mA | |
| | | Explosion protection | II 2(1) G EEx ib [ia] IIC T6 CE 0032 TÜV 01 ATEX 1689 | |
| | | Data retention | > 10 years (EEPROM) | |

| | |
|---------------------|---|
| EMC | Emitted interference: EN 61 326 Class B Immunity to interference: EN 61 326, EN 61 326/A1 |
| Temperature | Operating/environmental temp -20 to +55 °C Transport and storage temp -20 to +70 °C |
| Enclosure | Material: thermoplastic polyester, re- inforced (polybutylene terephthalate) Protection: IP 65 Color: bluish gray RAL 7031 |
| Cable glands | 3 breakthroughs for included cable glands 2 breakthroughs for cable glands, NPT 1/2 " or Rigid Metallic Conduit |
| Dimensions | See Dimension drawings, Pg. 7 ff |
| Weight | approx. 1 kg |

*) user defined 1) ± 1 count
2) with Pt 100 < 1K, with NTC > 100 °C < 1 K

EC-Type-Examination Certificate



Translation

EC-TYPE EXAMINATION CERTIFICATE

(1) **EC-TYPE EXAMINATION CERTIFICATE**

(2) Equipment or Protective System intended for use in potentially explosive atmospheres - **Directive 94/9/EC**

(3) EC-Type Examination Certificate Number

TÜV 01 ATEX 1689

(4) Equipment or Protective System: Transmitter type 22*1 X Cond

(5) Manufacturer: ProMinent Dosertechnik GmbH

(6) Address: D-69123 Heidelberg, Im Schuhmachergewann 5-11

(7) This equipment or protective system and any acceptable variation thereto is specified in the schedule to this certificate and the documents therein referred to.

(8) The TÜV Hannover/Sachsen-Anhalt e.V., TÜV Certification Body N° 0032 in accordance with Article 9 of the Council Directive 94/9/EC of March 23, 1994, certifies that this equipment or protective system has been found to comply with the Essential Health and Safety Requirements relating to the design and construction of equipment and protective systems intended for use in potentially explosive atmospheres given in Annex II to the Directive.

The examination and test results are recorded in confidential report N° 01 PX 06910.

(9) Compliance with the Essential Health and Safety Requirements has been assured by compliance with:

EN 50 014:1997 EN 50 020:1994

(10) If the sign "X" is placed after the certification number, it indicates that the equipment or protective system is subject to special conditions for safe use specified in the schedule to this certificate.

(11) This EC-TYPE EXAMINATION CERTIFICATE relates only to the design and construction of the specified equipment or protective system. If applicable, further requirements of this Directive apply to the manufacture and supply of this equipment or protective system.

(12) The marking of the equipment or protective system shall include the following:

 **II 2 (1) G EEx Ib [ia] IIC T6**

TÜV Hannover/Sachsen-Anhalt e.V.
TÜV CERT-Zertifizierungsstelle
Am TÜV 1
D-30519 Hannover

Hannover, 2001-03-14


Head of the Certification Body



This certificate may only be reproduced without any change, schedule included.
Excerpts or changes shall be allowed by the TÜV Hannover/Sachsen-Anhalt e.V.

page 1/3



(13)

SCHEDULE

(14) **EC-TYPE EXAMINATION CERTIFICATE N° TÜV 01 ATEX 1689**

(15) Description of equipment or protective system

The transmitter type 22*1 X Cond is used for the recognition and processing of electrochemical quantities.

The maximum permissible ambient temperature is 55°C.

Electrical data

Current loop.....in type of protection "Intrinsic Safety" EEx ib IIC
(terminals 10, 11) only for the connection to a certified intrinsically safe circuit
with the following maximum values:

$U_i = 30 \text{ V}$
 $I_i = 100 \text{ mA}$
 $P_i = 0,8 \text{ W}$
effective internal capacitance $C_i = 20 \text{ nF}$
effective internal inductance $L_i = 0,2 \text{ mH}$

Conductivity measuring loop....in type of protection "Intrinsic Safety" EEx ia IIC
(terminals 1, 2, 3, 4, 5) Maximum values:

$U_0 = 10 \text{ V}$
 $I_0 = 145 \text{ mA}$
 $P_0 = 145 \text{ mW}$
 $R_i = 34,5 \text{ } \Omega$
Characteristic: linear
effective internal capacitance $C_i = 3 \text{ nF}$
The effective internal inductance is negligibly small.
max. permissible external capacitance $C_e = 3 \text{ } \mu\text{F}$
max. permissible external inductance $L_e = 1 \text{ mH}$

Temperature measuring loop....in type of protection "Intrinsic Safety" EEx ia IIC
(terminals 7, 8) Maximum values:

$U_0 = 5 \text{ V}$
 $I_0 = 3,5 \text{ mA}$
 $P_0 = 5 \text{ mW}$
 $R_i = 1500 \text{ } \Omega$
Characteristic: linear
effective internal capacitance $C_i = 250 \text{ nF}$
The effective internal inductance is negligibly small.
max. permissible external capacitance $C_e = 100 \text{ } \mu\text{F}$
max. permissible external inductance $L_e = 1 \text{ H}$

14.03.2006

page 2/3



Schedule EC-type examination certificate N° TÜV 01 ATEX 1689

EP (PA) for the connection to the equipotential bonding system
(Terminal 9)

The current loop is safely galvanically separated from the conductivity measuring loop and the temperature measuring loop up to a voltage of 60 V. The conductivity measuring loop and the temperature measuring loop are galvanically connected.

(16) Test documents are listed in the test report No. 01 PX 06910.

(17) Special condition for safe use
none.

(18) Essential Health and Safety Requirements
no additional ones

Declaration of Conformity

EC Declaration of Conformity

We, **ProMinent Dosiertechnik GmbH
Im Schuhmachergewann 5 - 11
D - 69123 Heidelberg**

hereby declare that, on the basis of its functional concept and design and in the version brought into circulation by us, the product specified in the following complies with the relevant, fundamental safety and health stipulations laid down by EC directives.
Any modification to the product not approved by us will invalidate this declaration.

Product description : **Dulcometer transducer**

Product type : **2201 X Cond, 2201 X Condl**

Serial number : **see type identification plate on device**

Relevant EC regulations : **EC - EMC - regulation (89/336/EEC subsequently 92/31 EEC)
EC directive for devices in hazardous areas 94/9/EC**

Harmonised standards used, in particular : **DIN EN 61326, DIN EN 50014, DIN EN 50020**

National standards and other technical specifications used, in particular :

Date/manufacturer's signature :  **June 12, 2001**

The undersigned : **Dr Rainer V. Dulger, Executive Vice President R&D and Production**

ATE_Doku, EG-Konf_Erklärung

KE 2201 X Cond e 01-06-12.xls

12.06.01 10:29

Sensors

| | | |
|--|-----------------------------------|-----------------------------|
| Model LF 604 (2-electrode cell) by Regnault | | |
| Cell constant | 0.029 cm ⁻¹ | |
| Range | 0.02 – 5,000 μS/cm ¹) | |
| Material | Body | stainless steel 1.4571 |
| | Electrodes | stainless steel 1.4571 |
| Max. temperature | 120 °C | |
| Max. pressure | 25 bars: | sensor with external thread |
| | 16 bars: | sensor with flange PN 16 |
| | 10 bars: | all other versions |
| Temp probe | Pt 1000 | |
| Cable | Length | 5 m |
| | Connection wire end ferrule | |
| Dimensions | See dimension drawing fig. 11 | |

Observe installation clearances!


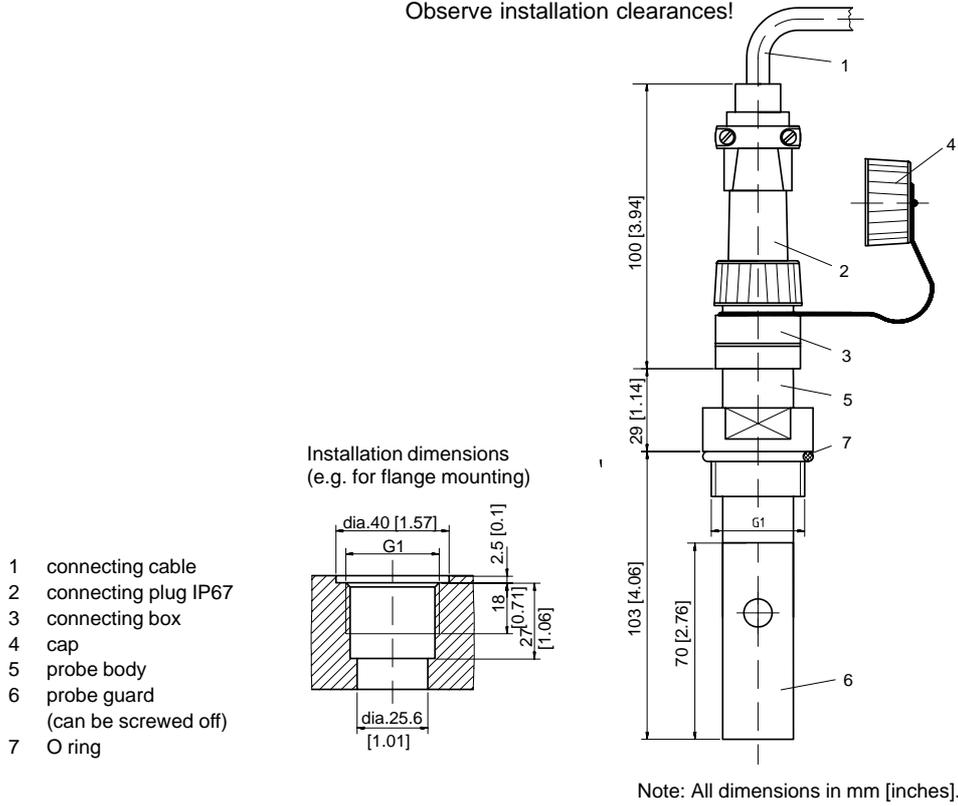


Fig. 11 Dimension drawing LF 604 2-electrode cell

Observe installation clearances!

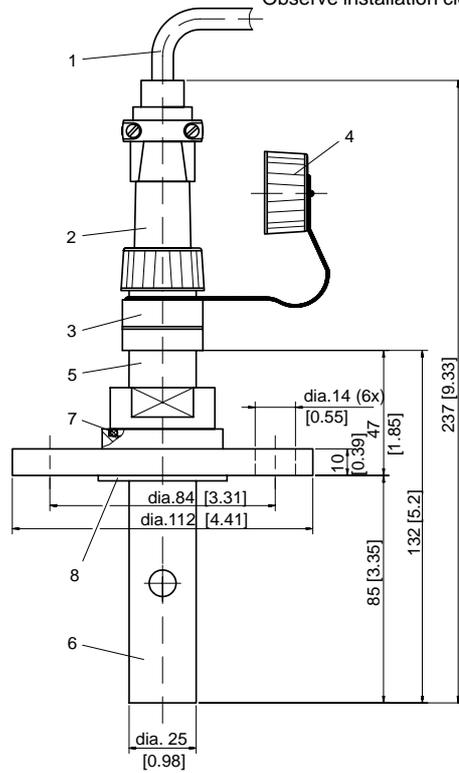

- 1 connecting cable
- 2 connecting plug IP67
- 3 connecting box
- 4 cap
- 5 probe body
- 6 probe guard
(can be screwed off)
- 7 O ring
- 8 flat gasket


Note: All dimensions in mm [inches].

Fig. 12 Dimension drawing LF 604 2-electrode cell with flange

Observe installation clearances!

min. 150 [5.91]

- 1 connecting cable
- 2 connecting plug
- 3 connecting box
- 4 cap
- 5 probe body
- 6 flow cell
- 7 wall mounting assembly
- 8 hole for M6 fastening screw

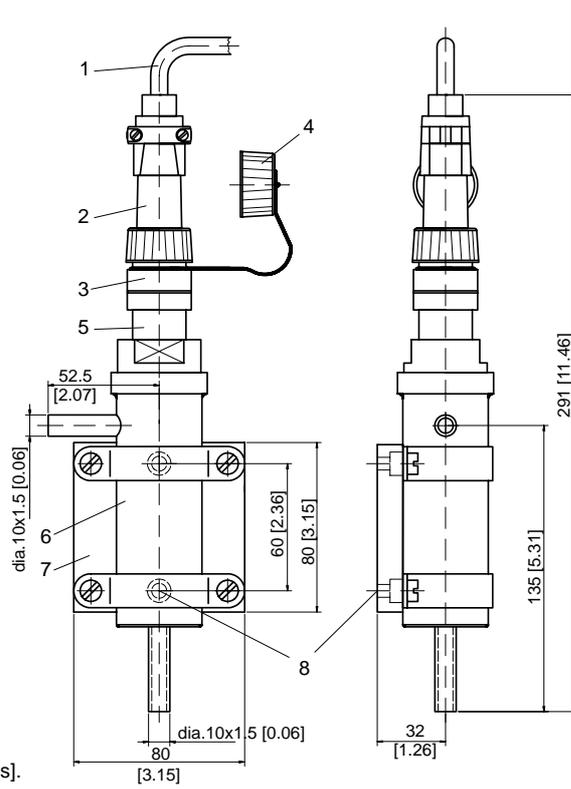

Note: All dimensions in mm [inches].

Fig. 13 Dimension drawing LF 604 2-electrode cell with flow-through fitting

Calibration Solutions

| Potassium Chloride Solutions | | | | Sodium Chloride Solutions | | | |
|----------------------------------|---------------|-----------|---------|----------------------------------|---------------|---------------|----------------|
| Electrical Conductivity in mS/cm | | | | Electrical Conductivity in mS/cm | | | |
| Temperature | Concentration | | | Temperature | Concentration | | |
| [°C] | 0.01 mol/l | 0.1 mol/l | 1 mol/l | [°C] | saturated*) | 0.1 mol/l(**) | 0.01 mol/l(**) |
| 0 | 0.776 | 7.15 | 65.41 | 0 | 134.5 | 5.786 | 0.631 |
| 5 | 0.896 | 8.22 | 74.14 | 1 | 138.6 | 5.965 | 0.651 |
| 10 | 1.020 | 9.33 | 83.19 | 2 | 142.7 | 6.145 | 0.671 |
| 15 | 1.147 | 10.48 | 92.52 | 3 | 146.9 | 6.327 | 0.692 |
| 16 | 1.173 | 10.72 | 94.41 | 4 | 151.2 | 6.510 | 0.712 |
| 17 | 1.199 | 10.95 | 96.31 | 5 | 155.5 | 6.695 | 0.733 |
| 18 | 1.225 | 11.19 | 98.22 | 6 | 159.9 | 6.881 | 0.754 |
| 19 | 1.251 | 11.43 | 100.14 | 7 | 164.3 | 7.068 | 0.775 |
| 20 | 1.278 | 11.67 | 102.07 | 8 | 168.8 | 7.257 | 0.796 |
| 21 | 1.305 | 11.91 | 104.00 | 9 | 173.4 | 7.447 | 0.818 |
| 22 | 1.332 | 12.15 | 105.94 | 10 | 177.9 | 7.638 | 0.839 |
| 23 | 1.359 | 12.39 | 107.89 | 11 | 182.6 | 7.831 | 0.861 |
| 24 | 1.386 | 12.64 | 109.84 | 12 | 187.2 | 8.025 | 0.883 |
| 25 | 1.413 | 12.88 | 111.80 | 13 | 191.9 | 8.221 | 0.905 |
| 26 | 1.441 | 13.13 | 113.77 | 14 | 196.7 | 8.418 | 0.927 |
| 27 | 1.468 | 13.37 | 115.74 | 15 | 201.5 | 8.617 | 0.950 |
| 28 | 1.496 | 13.62 | | 16 | 206.3 | 8.816 | 0.972 |
| 29 | 1.524 | 13.87 | | 17 | 211.2 | 9.018 | 0.995 |
| 30 | 1.552 | 14.12 | | 18 | 216.1 | 9.221 | 1.018 |
| 31 | 1.581 | 14.37 | | 19 | 221.0 | 9.425 | 1.041 |
| 32 | 1.609 | 14.62 | | 20 | 226.0 | 9.631 | 1.064 |
| 33 | 1.638 | 14.88 | | 21 | 231.0 | 9.838 | 1.087 |
| 34 | 1.667 | 15.13 | | 22 | 236.1 | 10.047 | 1.111 |
| 35 | 1.696 | 15.39 | | 23 | 241.1 | 10.258 | 1.135 |
| 36 | | 15.64 | | 24 | 246.2 | 10.469 | 1.159 |
| | | | | 25 | 251.3 | 10.683 | 1.183 |
| | | | | 26 | 256.5 | 10.898 | 1.207 |
| | | | | 27 | 261.6 | 11.114 | 1.232 |
| | | | | 28 | 266.9 | 11.332 | 1.256 |
| | | | | 29 | 272.1 | 11.552 | 1.281 |
| | | | | 30 | 277.4 | 11.773 | 1.306 |
| | | | | 31 | 282.7 | 11.995 | 1.331 |
| | | | | 32 | 288.0 | 12.220 | 1.357 |
| | | | | 33 | 293.3 | 12.445 | 1.382 |
| | | | | 34 | 298.7 | 12.673 | 1.408 |
| | | | | 35 | 304.1 | 12.902 | 1.434 |
| | | | | 36 | 309.5 | 13.132 | 1.460 |

Data source: K. H. Hellwege (Editor), H. Landolt, R. Börnstein: Zahlenwerte und Funktionen Volume 2, Part. Volume 6

Data source: *) K. H. Hellwege (Editor), H. Landolt, R. Börnstein: Zahlenwerte und Funktionen Volume 2, Part. Volume 6

**) Test solutions calculated according to IEC 746-3

Index

- ☺ ☹, 23
- 22 mA signal for alarm, 16, 23
configuring, 18
- A**
- Alarm, 16
response time, 23
- Alarm contact, 23
- Alarm LED, 23
- Alarm via loop current, 16, 23
configuring, 18
- Assembly, 6
- C**
- Cal info, 22, 25
- Calibration, 19
input of cell constant, 19
temp probe adjustment, 21
with calibration solution, 20
- Calibration data, display, 25
- Calibration solutions, 36
- Certificate of Conformity, 30
- Cleaning, 26
- Conductivity measurement, 22
- Configuration, 17
- Connecting, lines, 9
- Connecting cable, fixing, 9
- Current characteristic, configuring, 18
- Current loop
Hold state, 18
Hold value, 18
- Current source, 25
- D**
- Declaration of Conformity, 33
- Diagnostics functions, 25
- Dimension drawings, 7
- Display, 14
- E**
- EC Type Examination Certificate, 30
- Error info, 22, 23, 25
- Error message, last, 22, 23, 25
- Error message via loop current, 16, 23
configuring, 18
- Error messages, 23–26
- G**
- GainCheck, 15, 25
- H**
- Hold state, 22
- I**
- Installation, 11
- Instrument self-test
automatic, 15
manual, 15
- K**
- Keypad, 14
- L**
- Loop current, 16
display, instantaneous, 25
frozen, 22
- M**
- Maintenance, 26
- Measuring mode, 22
- Messages, Sensoface, 23
- Mode code, 4
- Mounting diagram, 7
- O**
- Outputs, 16
- P**
- Packing list, 6

| | | |
|--|--|---------------------------|
| Pipe mount kit, 8 | Sensor LF 604 dimension drawing, 35 specifications, 34 | Stripping lengths, 9 |
| Process variable, configuring, 17 | | T |
| Product line, 27 | | |
| Protective hood, 8 | Sensor monitoring, Sensoface, 23 | Terminals, pulling out, 9 |
| S | | Test mode, 25 |
| Safety precautions, 3 | Sensors, 34 configuring, 17 monitoring, 15 | U |
| Self-test automatic, 25 manual, 25 | Smiley, 23 | User Interface, 13 |
| Sensocheck, on or off, 18 | Software version, display, 15, 25 | W |
| Sensoface, 15, 23 diagnostics, 23 messages, 23 | Specifications, 28 | Wiring example, 12 |

**Addresses and delivery information
from the manufacturer:**

ProMinent Dosiertechnik GmbH
Im Schuhmachergewann 5–11
D-69123 Heidelberg

Postfach 10 17 60
D-69007 Heidelberg – Germany

Phone: +49 (06221) 842-0
Fax: +49 (06221) 842-419
info@prominent.de
www.prominent.de